

See for similar files: <http://www.ps.bam.de/FE95/FE95.HTM>  
 Information and Order: <http://www.ps.bam.de> Version 2.0, io=5,0; iORS; oORS, CIELAB

C  
 $LAB^*$

M  
 $LAB^*$

Y  
 $LAB^*$

N  
 $LAB^*$

O  
 $LAB^*$

L  
 $LAB^*$

V  
 $LAB^*$

N  
 $LAB^*$

BAM registration: 20030101-FE95/10L/L95E00FP.PS/.PDF BAM material: code=rha4ta  
 application for measurement of monitor (Yr=2.5) and printer output

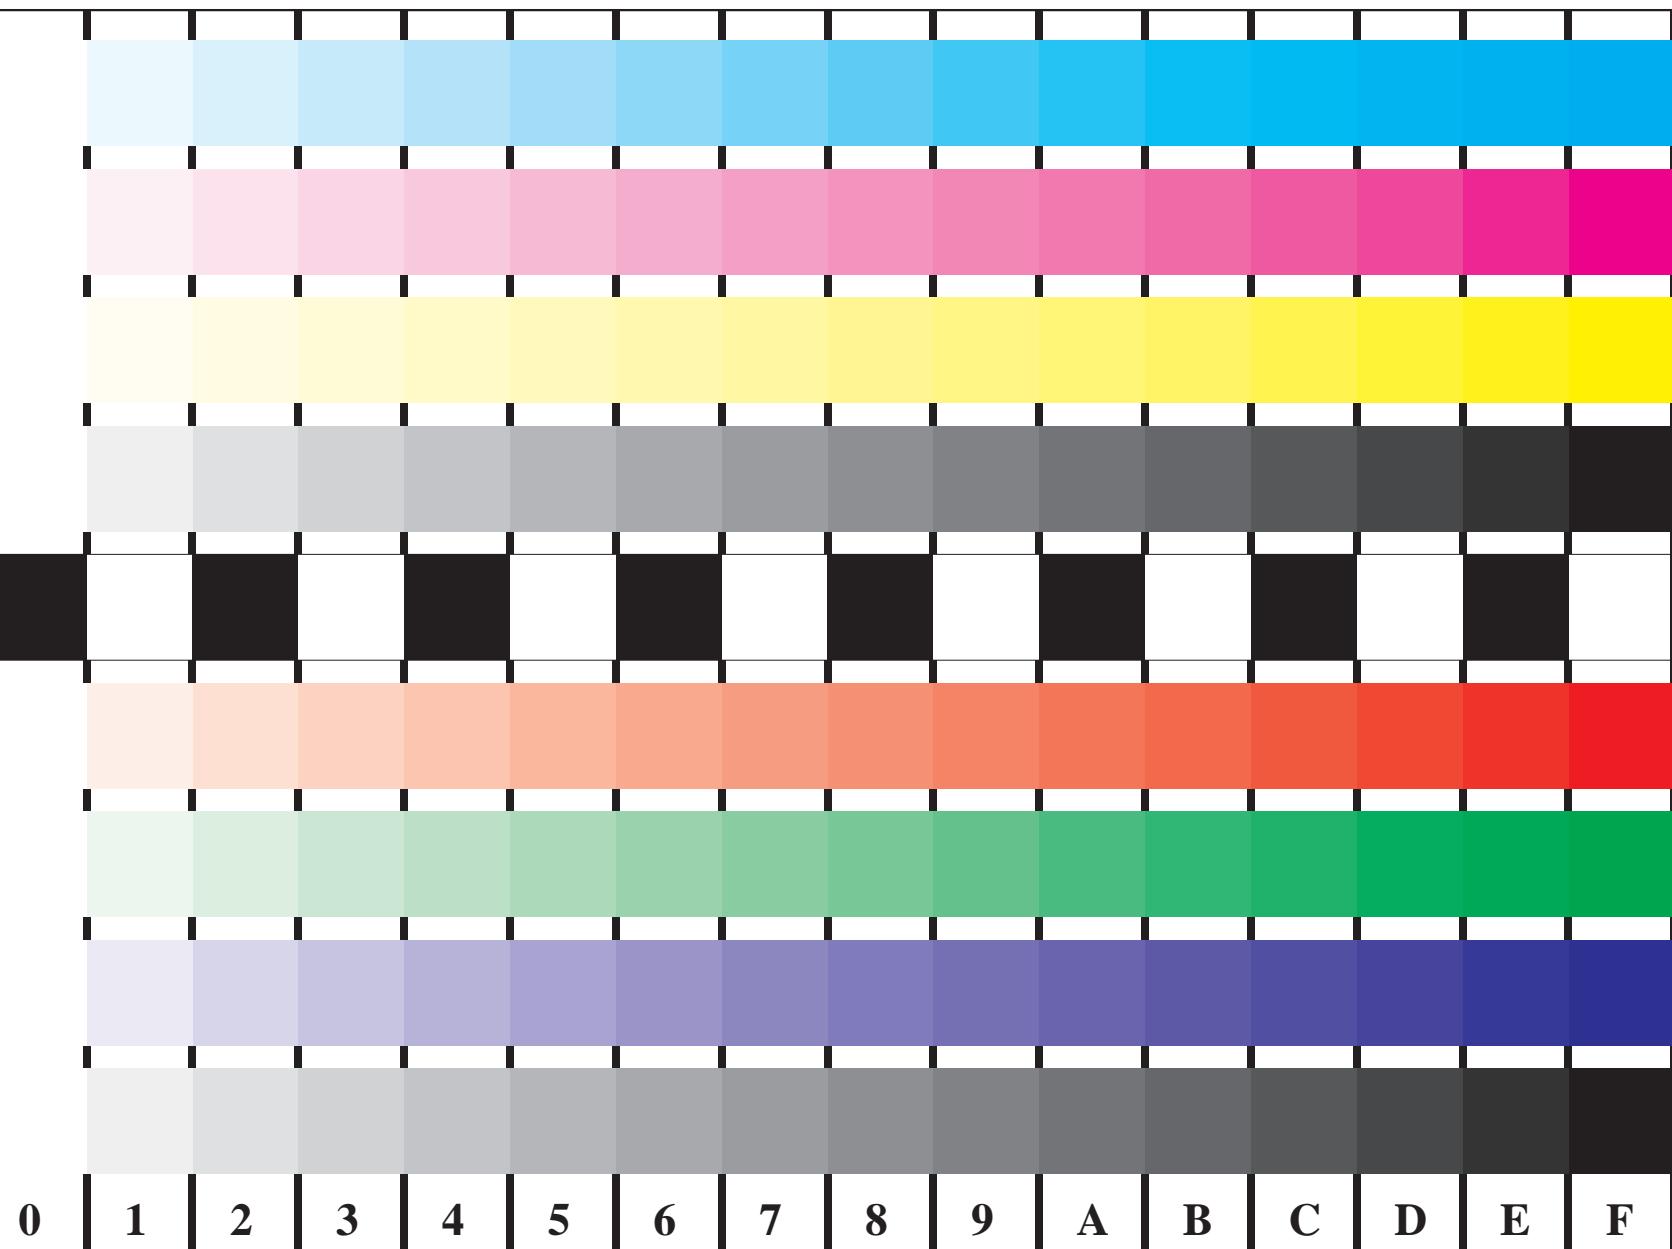


Figure B4 and D4 of the ISO/IEC-test charts no. 2 and 4; 16 visual equidistant steps of colour series; Use of the PS operator  $LAB^* setcolor$




Fig. B4 of ISO/IEC-test chart 2 and  
 Fig. D4 of ISO/IEC-test chart no. 4;

ISO/IEC 15775 and  
 TR ISO/IEC 24705;

input:  $LAB^* setcolor$   
 output:  $cmy0*/000n* setcmykcolor$

