

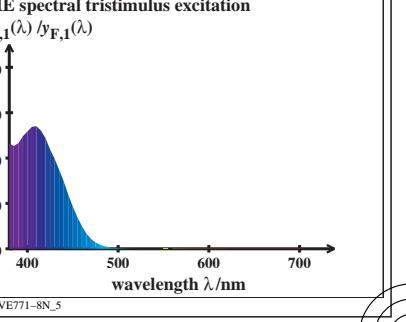
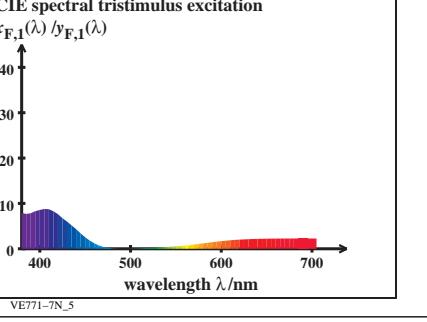
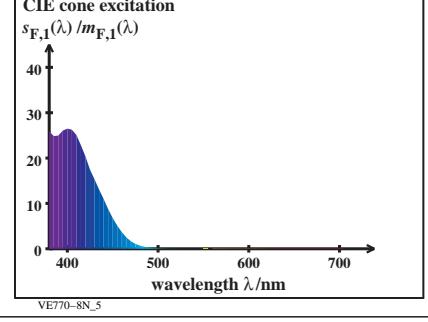
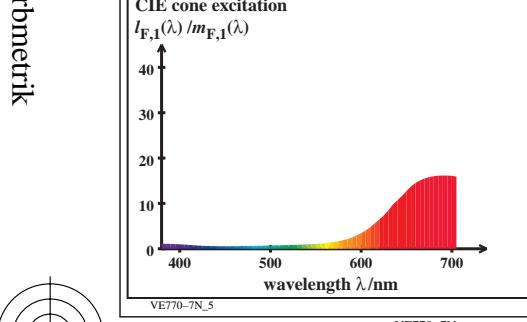
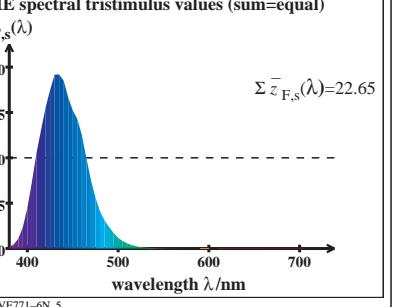
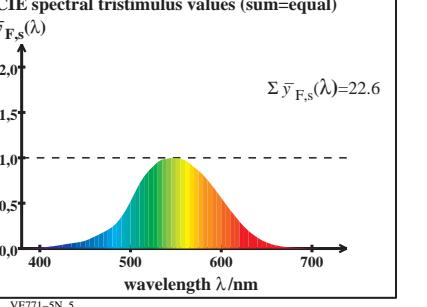
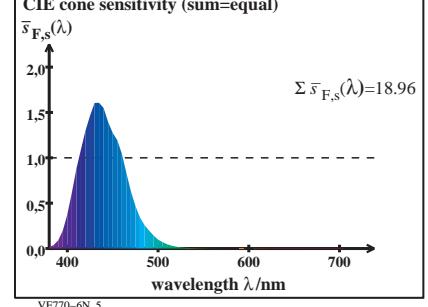
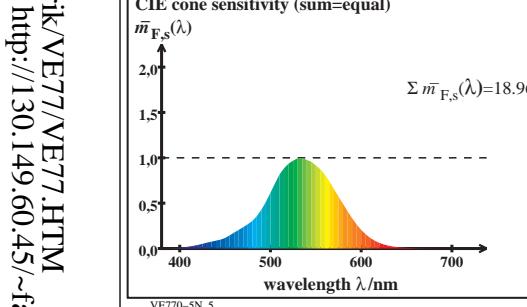
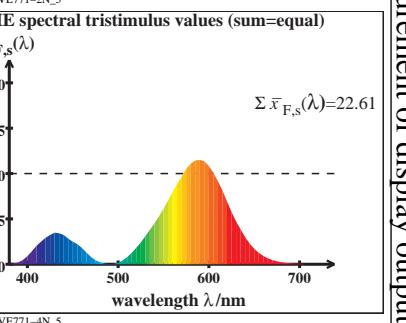
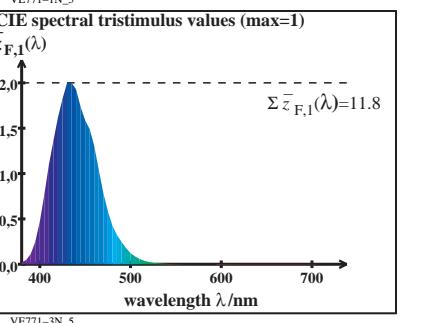
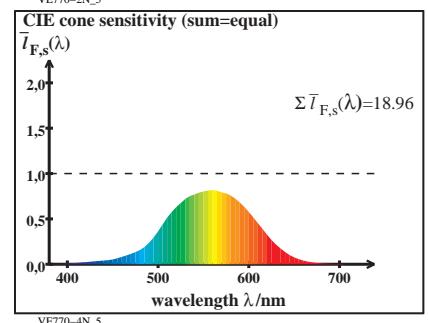
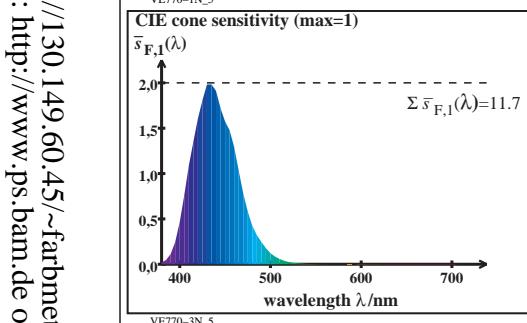
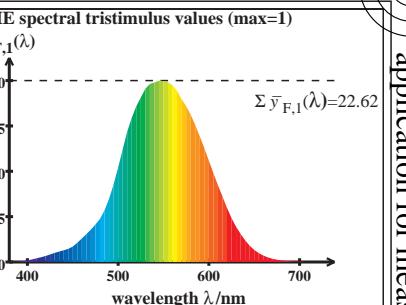
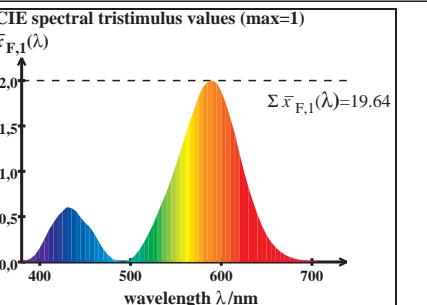


see similar files: <http://130.149.60.45/~farbmertik/VE77/VE77L0NA.TXT/.PS>  
 technical information: <http://www.ps.bam.de> or <http://130.149.60.45/~farbmertik>

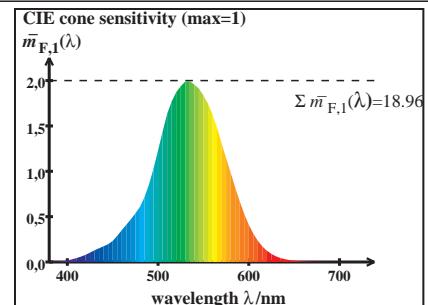

TUB-test chart VE77; CIE fundamental (F) colorimetry  
 Cone sensitivity and excitation, and spectral tristimulus values for CIE illuminant E; linear data

input: w/rgb/cmyk -> w/rgb/cmyk-  
 -> CIE fundamental (F) colorimetry

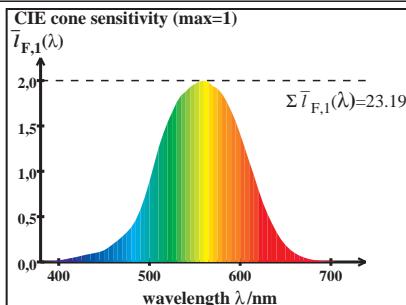